




CoLink NeoFuse[®]

MIS Plating System

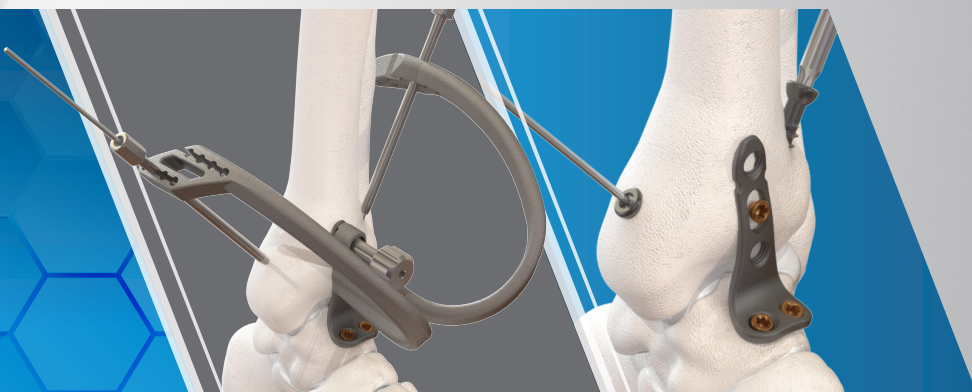

SURGICAL TECHNIQUE

Table of Contents

Tray Layouts

MIS Tray Layout	3
Standard Tray Layout	3

Product Overview

Indications for Use	4
Plate Configurations	4
Associated Screws	4

Surgical Pearls

Sizing Plate Screw Length	5
Screw-Specific Insertion Techniques	5

Associated Drill Guides and Targeting Guide

Screw Preparation Options	6
Targeting Guide	6

Plate-Specific Insertion Techniques

Joint Preparation	7
Trialing	7
Provisional Fixation	7
Talar Screws	7
Oblong Tibial Hole	8
Medial & Lateral Posterior Fixation Screws	8
Remaining Tibial Screws	9
Finalize Construct & Close	9

Ordering Information

Screws	10
CoLink® NeoFuse MIS Plates	12
Sterile Instruments	12

CoLink® NeoFuse MIS Plating System

MIS Instrument Tray


P02 N0002



DESCRIPTION	CATALOG NO.	QTY
1 MIS Plate Targeting Guide, K-wire Guide	P02 N0231	2
2 MIS Plate Targeting Guide	P02 N0171	1
3 MIS Plate, Trial	P02 N1301	1
4 MIS Plate Targeting Guide, Guide Screw	P02 N0221	2

Standard Instrument Tray

P02 N0001

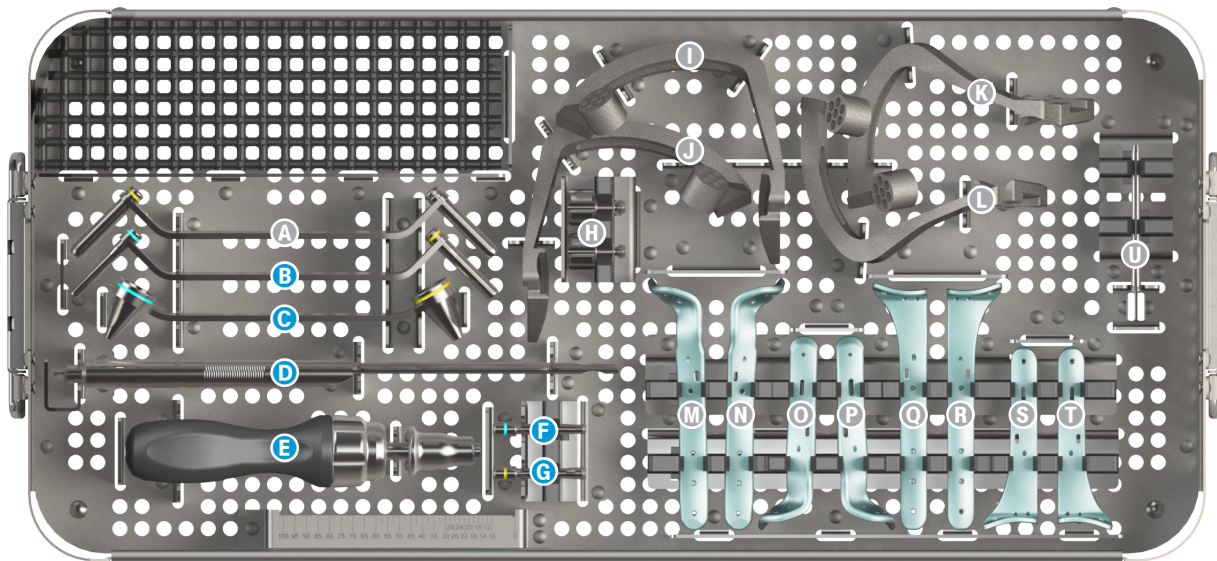

● Used in MIS Procedure ● Not Used

DESCRIPTION	CATALOG NO.	QTY	DESCRIPTION	CATALOG NO.	QTY
A Transverse Drill Guide, 4.5 Screws, Assembly	P02 N0051	1	L Targeting Guide, Anterior, Left	P02 N0071	1
B NL Drill Guide, 2.5,3.2 Assembly	P02 N0031	1	M Anterolateral Plate, 5H, Right, Trial	P02 N1201	1
C Variable Drill Guide, 2.5, 3.2 Assembly	P02 N0021	1	N Anterolateral Plate, 5H, Left, Trial	P02 N1202	1
D Screw Depth Gauge, 0-100mm	P02 N0041	1	O Anterolateral Plate, 3H, Left, Trial	P02 N1204	1
E Ratcheting Handle, AO, QC	P04 N0063	1	P Anterolateral Plate, 3H, Right, Trial	P02 N1203	1
F Afx, Locking Drill Guide 2.5	P07 N0011	2	Q Anterior Plate, 5H, Right, Trial	P02 N1101	1
G Ankle Fusion Locking Drill Guide 3.2	P02 N0011	2	R Anterior Plate, 5H, Left, Trial	P02 N1102	1
H Targeting Guide, Screws	P02 N0101	2	S Anterior Plate, 3H, Left, Trial	P02 N1104	1
I Targeting Guide, Anterolateral, Right	P02 N0081	1	T Anterior Plate, 3H, Right, Trial	P02 N1103	1
J Targeting Guide, Anterolateral, Left	P02 N0091	1	U Targeting Guide, K-wire Guide	P02 N0111	2
K Targeting Guide, Anterior, Right	P02 N0061	1			

CoLink® NeoFuse MIS Plating System

Product Overview

The **CoLink® NeoFuse MIS Plating System** is a line extension to the current CoLink® plating system offerings. The CoLink® NeoFuse MIS Plating System features two symmetrical MIS Plates. A symmetrical Targeting Guide is provided for placement of posterior transverse compression and neutralization screws outside of the plate for added compression and stability to the joint.

- » MIS Plate, Standard
- » MIS Plate, 3.5mm Talar Holes

Associated screws are CoLink® 3.5mm Locking, Non-Locking and Variable Angle Locking Screws, CoLink® 4.5mm Locking, Non-Locking, and Variable Angle Locking Screws, and NEW CoLink® 5.0mm Non-Locking Cancellous Screws which may be used in place of 4.5mm CoLink Non-Locking Screws based on surgeon preference. CoLag® 6.7mm Compression and Neutralization Screws are used as transverse screws with these plates.

All implants are provided sterile packaged. The system utilizes a set of sterile and reusable instruments, which includes a trial plate for determination of proper placement prior to selecting the desired packaged plate implant. Other standard orthopedic operating instrumentation may be required to perform the procedures.

Indications for Use


The CoLink® NeoFuse MIS Plating System is indicated for anterior fixation of ankle arthrodesis and fractures, including the distal tibia and talus. The addition of a posterior compression screw and fully threaded screw through the tibiotalar joint (example CoLag® 6.7mm screw) are required for ankle fusion procedure.

See package insert for more information, including contraindications, warnings, and precautions.

Plate Configurations




Associated Screws

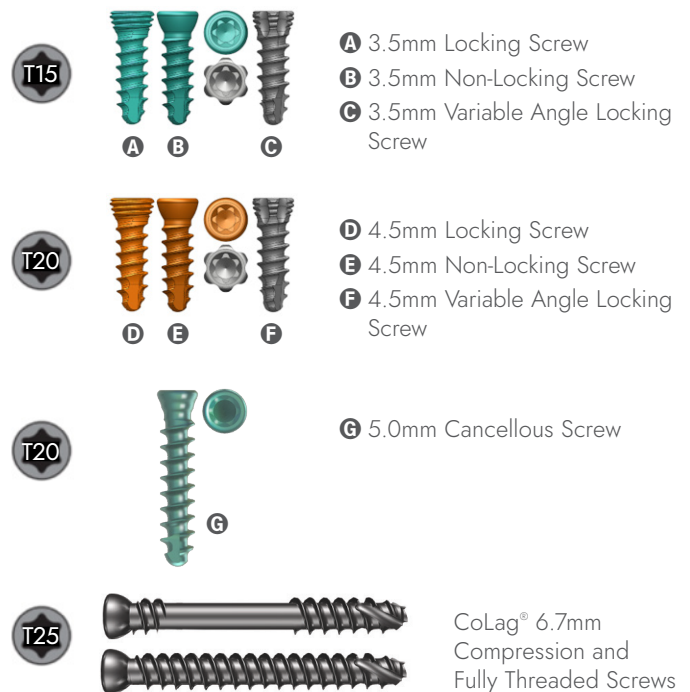

CoLink® NeoFuse MIS Plating System

Surgical Pearls

Sizing Plate Screw Length



Place the end of the Depth Gauge into the screw hole of the chosen plate, upon completion of screw hole preparation. Rest the end of the Depth Gauge against the bone and insert the probe through the prepared screw hole. Pull back on

the slide to hook the far cortex with the tip of the probe and read the measurement on the body of the Depth Gauge.

Screw-Specific Insertion Techniques



3.5mm Non-Locking Cortical

Using the 2.5mm end of the 2.5/3.2mm Non-Locking Drill Guide in conjunction with the 2.5mm Drill, drill through the screw hole taking care not to violate critical soft tissue or joint space. Depth measurement may be read off the markings on the Drill relative to the top of the Drill Guide. Non-Locking Screws may be placed up to 15 degrees in any direction off the standard axis of the screw hole. Depth measurement may also be determined using the Depth Gauge (see section on Sizing Plate Screw Length). Select the corresponding screw size and place the Screw with the supplied T15 driver and AO Ratchet Handle until fully seated.



3.5mm Locking Cortical Screw

Thread the 2.5mm Afx Locking Drill Guide into the plate and use the 2.5mm Drill to drill through the screw hole taking care not to violate critical soft tissue or joint space. Depth measurement may be read off the markings on the Drill relative to the top of the Drill Guide. Depth measurement may also be determined using the Depth Gauge (see section on Sizing Screw Length). Select the corresponding screw size and place the Screw with the supplied T15 driver and AO Ratchet Handle until fully seated.



3.5mm Variable Angle Locking Screw

Place the 2.5mm end of the 2.5/3.2mm Variable Angle Drill Guide into the plate in conjunction with the 2.5mm Drill, drill through the screw hole taking care not to violate critical soft tissue or joint space. Remove the Drill Guide and take a depth measurement using the Depth Gauge (see section on Sizing Screw Length). Select the corresponding screw size and place the Screw with the supplied T15 driver and AO Ratchet Handle until fully seated.



4.5mm Locking Cortical Screw

Thread the 3.2mm Ankle Fusion System Locking Drill Guide into the plate and use the 3.2mm Drill to drill through the screw hole taking care not to violate critical soft tissue or joint space. Depth measurement may be read off the markings on the Drill relative to the top of the Drill Guide. Depth measurement may also be determined using the Depth Gauge (see section on Sizing Screw

Length). Select the corresponding screw size and place the Screw with the supplied T20 driver and AO Ratchet Handle until fully seated.



4.5mm Non-Locking Cortical Screw

Using the 3.2mm end of the 2.5/3.2mm Non-Locking Drill Guide along with the 3.2mm Drill, drill through the screw hole taking care not to violate critical soft tissue or joint space. Depth measurement may be read off the markings on the Drill relative to the top of the Drill Guide. Non-Locking Screws may be placed up to 15 degrees in any direction off the standard axis of the screw hole. Depth measurement may also be determined using the Depth Gauge (see section on Sizing Screw Length). Select the corresponding screw size and place the Screw with the supplied T20 driver and AO Ratchet Handle until fully seated.




4.5mm Variable Angle Locking Screw

Place the 3.2mm end of the 2.5/3.2mm Variable Angle Drill Guide into the plate in conjunction with the 3.2mm Drill, drill through the screw hole taking care not to violate critical soft tissue or joint space. Remove the Drill Guide and take a depth measurement using the Depth Gauge (see section on Sizing Screw Length). Select the corresponding screw size and place the Screw with the supplied T20 driver and AO Ratchet Handle until fully seated.



5.0mm Non-Locking Cancellous Screw

Using the 3.2mm end of the 2.5/3.2mm Non-Locking Drill Guide along with the 3.2mm Drill, drill through the screw hole taking care not to violate critical soft tissue or joint space. Depth measurement may be read off the markings on the drill relative to the top of the drill guide. Non-Locking Cancellous Screws may be placed up to 15 degrees in any direction off the standard axis of the screw hole. Depth measurement may also be determined using the Depth Gauge (see section on Sizing Screw Length). Select the corresponding screw size and place the Screw with the supplied T20 driver and AO Ratchet Handle until fully seated. The 5.0 Non-Locking Cancellous Screw is a suitable replacement for the previously described 4.5mm Non-Locking Cortical Screw according to surgeon preference.




6.7mm CoLag® Screws (Compression and Neutralization)

Use the MIS Targeting Guide, Guide Screw, and K-wire Guides to position 0.079 X 9" single-trocar K-Wires across the joint. Remove the Targeting Guide and K-wire Guides. After the K-wires are positioned, slide the provided Screw Sizer over each K-wire to measure the appropriate depth to drill. Use the provided 4.8mm Cannulated Drill to drill to the measured depth over the K-wires, then remove the Drill. Select the corresponding screw size and place either a Compression or Neutralization Screw with a cannulated T25 driver and AO Ratchet Handle until fully seated.


CoLink® NeoFuse MIS Plating System

Associated Drill Guides and Targeting Guides


Screw Preparation Options

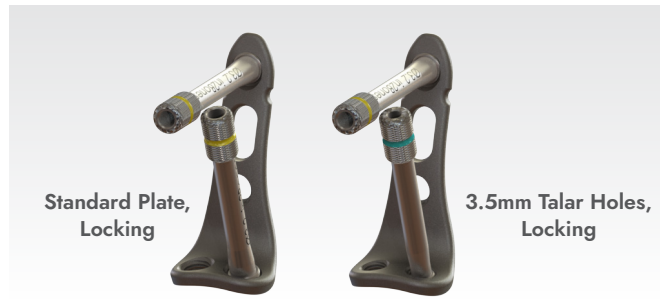

2.5mm and 3.2mm Locking Drill Guides are provided for on-axis drilling for 3.5 and 4.5mm Locking screws, respectively.

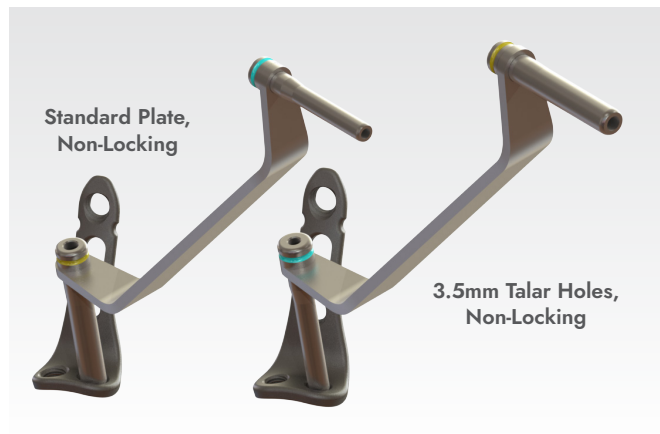

A 2.5/3.2mm Non-Locking Drill Guide is provided for off-axis drilling for 3.5 and 4.5mm Non-Locking Screws.

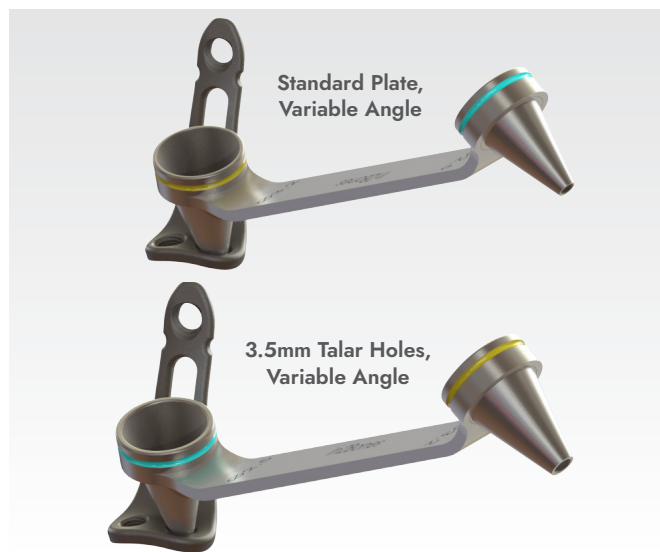

A 2.5/3.2mm Variable Angle Non-Locking Drill Guide is provided for off-axis drilling for 3.5mm and 4.5mm Variable Angle Screws with 30° of variability.

Targeting Guide



A symmetrical Targeting Guide is provided to enable targeting of the medial and lateral 6.7mm CoLag® Screws for additional fixation. Compression and Neutralization Screws are available. The Guide is designed to provide screw vectors that avoid on-axis plate screws.

CoLink® NeoFuse MIS Plating System

Surgical Technique

Joint Preparation

Remove any osteophytes that may interfere with the placement of the CoLink® NeoFuse MIS Plates and prepare the ankle joint using flat or resurfacing cuts per surgeon preference. If desired, temporary fixation of the bones may be obtained using K-wires.

Note: Fluoroscopic verification is recommended for each step of the procedure.

Trialing

Use the provided Trial to establish the appropriate plate configuration and position on the tibia and talus. Temporary fixation of the Trial may be obtained using the provided Olive Wires to allow fluoroscopic views while retaining the position of the Trial. **Figure 1**

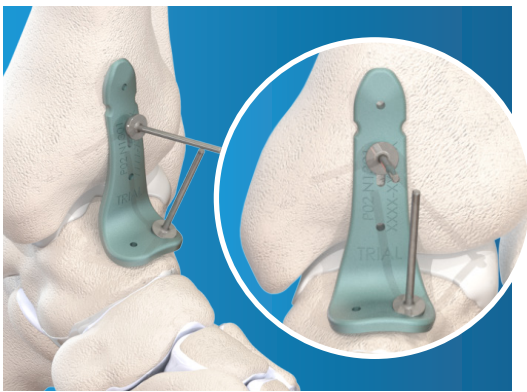


Figure 1. Trialing

Provisional Fixation

Place the chosen plate configuration onto the bone, using fluoroscopic views to verify alignment and proper positioning. Use two Olive Wires to secure the plate to the bone: one in the proximal aspect of the oblong tibial hole **A** and the second in one of the talar screw holes **B**. **Figure 2**



Figure 2. Provisional Fixation

Talar Screws

For the MIS Plate, Standard (Shown Throughout):

Using the 3.2x130mm Drill and the 3.2mm Locking Drill Guide or 3.2mm Variable Angle Drill Guide, drill for the first talar screw until contacting the 2nd cortical wall **A**. The appropriate screw length may be read from the calibrated Drill relative to the top of the Locking Drill Guide or measured using the Depth Gauge.

Select the appropriate 4.5mm Screw and seat it securely to the plate using the T20 Driver and Ratcheting AO QC Handle.

Remove the talar Olive Wire, then repeat the above steps for the remaining talar screws **B**. **Figure 3**

For the MIS Plate, 3.5mm Talar Holes:

Using the 2.5x60mm Drill and the 2.5mm Locking Drill Guide or 2.5mm Variable Angle Drill Guide, drill for the first talar screw until contacting the 2nd cortical wall. The appropriate screw length may be read from the calibrated Drill relative to the top of the Locking Drill Guide or measured using the Depth Gauge.

Select the appropriate 3.5mm Screw and seat it securely to the plate using the T15 Driver and Ratcheting AO QC Handle.

Remove the talar Olive Wire, then repeat the above steps for the remaining talar screws.



Figure 3. Prepare & Seat Talar Screws

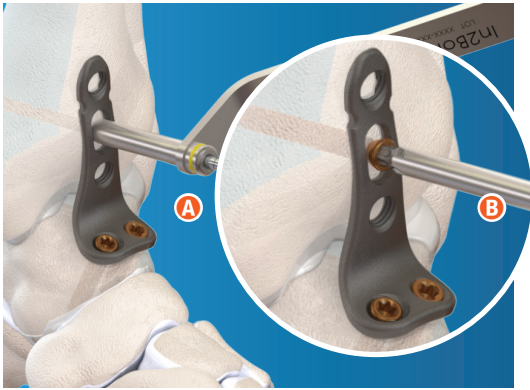


Figure 4. Prepare & Provisionally Seat Tibial Oblong Hole

Oblong Tibial Hole

Place the 4.5mm end of the Non-Locking Drill Guide in the proximal extent of the oblong tibial screw hole **A**. Prepare the screw hole using the 3.2x130mm Drill, taking care to reach the 2nd cortex.

Read the appropriate screw length from the calibrated Drill relative to the Drill Guide or measure using the Depth Gauge.

Select the appropriate 4.5mm Non-Locking Screw and provisionally seat the Screw to the plate using the T20 Driver and Ratcheting AO QC Handle **B**.

Figure 4

Note: Final seating of this Screw will be performed at a later step, allowing for translation of the Plate relative to the anterior aspect of the tibia resulting from the insertion of the CoLag® Compression and Neutralization Screws across the tibiotalar joint.



Figure 5. Assembly of Targeting Guide

Medial & Lateral Posterior Fixation Screws

Assemble the MIS Targeting Guide to the selected plate using the MIS Targeting Guide Screw, tightening until secure. **Figure 5**

Place K-wire Guides into the guide holes on the Targeting Guide which correspond to the desired screw trajectories for one CoLag® 6.7mm Compression Screw and one CoLag 6.7mm Neutralization Screw. Then, insert 0.079 X 9" K-wires through the K-wire Guides and across the joint up to the lateral process and the medial process of the talus. **Figure 6**

Fluoroscopic views may be taken to confirm K-wire placement and the desired trajectories.

Note: Care should be taken not to cross beyond the far cortex with each K-wire.

Remove the K-wire Guides from the Targeting Guide and disengage the Targeting Guide from the Plate by turning the Guide Screw counterclockwise.

Remove the Targeting Guide from the surgical field. **Figure 7**

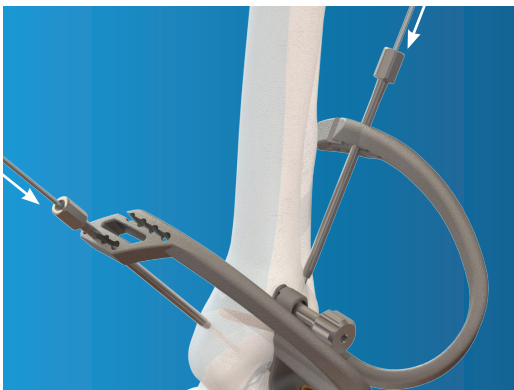


Figure 6. Place Medial & Lateral Wires Through Guide

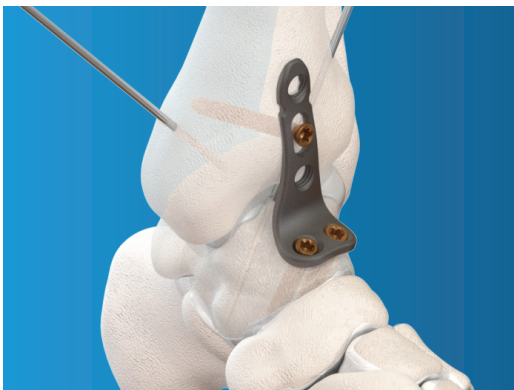


Figure 7. Remove Targeting Guide



Figure 8. Measure for 6.7mm CoLag® Screws

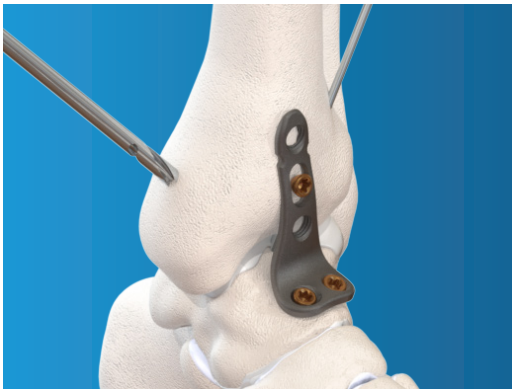


Figure 9. Drill for 6.7mm CoLag® Screws

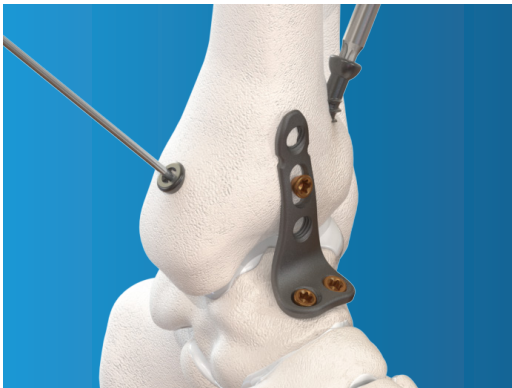


Figure 10. Seat CoLag® Screws

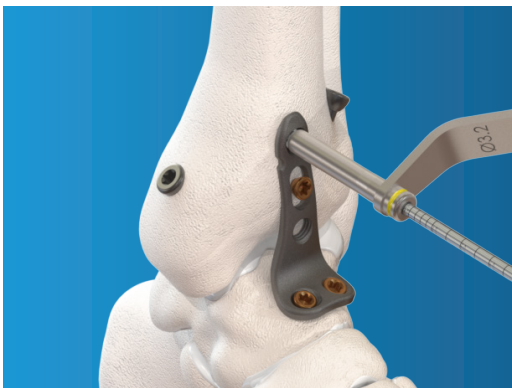


Figure 11. Prepare & Seat Remaining Tibial Screws

Assemble the Lag Screw Sizer over the 0.079 X 9" K-wires to assess the appropriate screw lengths. **Figure 8**

Important: A single CoLag® 6.7mm Compression Screw, and a single CoLag® 6.7mm Neutralization Screw should be placed with this construct. The decision on which screw is inserted medially and laterally should be made based on surgeon expertise and patient anatomy during the procedure. It is critical to note the K-wire chosen to correspond with each Screw during the measurement step to ensure the appropriate length of each Screw type is retrieved for implantation.

Using the 4.8mm Cannulated Drill, prepare pilot holes at the appropriate depths as determined using the Lag Screw Sizer. **Figure 9**

Remove the Drill, leaving the K-wires in place.

Assemble the selected CoLag® 6.7mm Compression Screw over the intended K-wire and seat to the bone using a T25 AO QC Driver and Ratcheting Handle to compress the joint. Follow with the selected CoLag® 6.7mm Neutralization Screw over the remaining K-wire. **Figure 10**

Remove the K-wires.

Remaining Tibial Screws

Using the 3.2x130mm Drill and the Drill Guide corresponding to the desired 4.5mm CoLink® Screw (Locking, Non-Locking, or Variable Angle), or 5.0mm CoLink® Non-Locking Cancellous Screw, prepare the remaining tibial screw holes until contacting the 2nd cortical wall. **Figure 11**

Insert the tip of the Depth Gauge into each of the prepared screw holes and measure the screw length, taking care to place the tip of the depth gauge at the bottom of the plate when measuring.

Select the corresponding screws and securely seat them to the plate using the T20 Driver and Ratcheting AO QC Handle.

Finalize Construct & Close

Perform final seating of the 4.5mm Non-Locking Screw in the oblong tibial plate hole to complete the construct. **Figure 12**

Close the incision per surgeon preference.




Figure 12. Tighten Screw in Oblong Hole & Complete Construct

CoLink® NeoFuse MIS Plating System

Compatible Screw Options

CoLink® Afx 3.5mm Diameter Screws (Sold Separately)

CATALOG NO.	DESCRIPTION	LENGTH
P73 ST010	CoLink® Afx Ø3.5 Low-Pro Cortical Screw	10mm
P73 ST012	CoLink® Afx Ø3.5 Low-Pro Cortical Screw	12mm
P73 ST014	CoLink® Afx Ø3.5 Low-Pro Cortical Screw	14mm
P73 ST016	CoLink® Afx Ø3.5 Low-Pro Cortical Screw	16mm
P73 ST018	CoLink® Afx Ø3.5 Low-Pro Cortical Screw	18mm
P73 ST020	CoLink® Afx Ø3.5 Low-Pro Cortical Screw	20mm
P73 ST022	CoLink® Afx Ø3.5 Low-Pro Cortical Screw	22mm
P73 ST024	CoLink® Afx Ø3.5 Low-Pro Cortical Screw	24mm
P73 ST026	CoLink® Afx Ø3.5 Low-Pro Cortical Screw	26mm
P73 ST028	CoLink® Afx Ø3.5 Low-Pro Cortical Screw	28mm
P73 ST030	CoLink® Afx Ø3.5 Low-Pro Cortical Screw	30mm
P73 ST032	CoLink® Afx Ø3.5 Low-Pro Cortical Screw	32mm
P73 ST034	CoLink® Afx Ø3.5 Low-Pro Cortical Screw	34mm
P73 ST036	CoLink® Afx Ø3.5 Low-Pro Cortical Screw	36mm
P73 ST038	CoLink® Afx Ø3.5 Low-Pro Cortical Screw	38mm
P73 ST040	CoLink® Afx Ø3.5 Low-Pro Cortical Screw	40mm
P73 ST042	CoLink® Afx Ø3.5 Low-Pro Cortical Screw	42.5mm
P73 ST045	CoLink® Afx Ø3.5 Low-Pro Cortical Screw	45mm
P73 ST047	CoLink® Afx Ø3.5 Low-Pro Cortical Screw	47.5mm
P73 ST050	CoLink® Afx Ø3.5 Low-Pro Cortical Screw	50mm
P73 ST052	CoLink® Afx Ø3.5 Low-Pro Cortical Screw	52.5mm
P73 ST055	CoLink® Afx Ø3.5 Low-Pro Cortical Screw	55mm
P73 ST057	CoLink® Afx Ø3.5 Low-Pro Cortical Screw	57.5mm
P73 ST060	CoLink® Afx Ø3.5 Low-Pro Cortical Screw	60mm
P73 ST110	CoLink® Afx Ø3.5 Locking Screw	10mm
P73 ST112	CoLink® Afx Ø3.5 Locking Screw	12mm
P73 ST114	CoLink® Afx Ø3.5 Locking Screw	14mm
P73 ST116	CoLink® Afx Ø3.5 Locking Screw	16mm
P73 ST118	CoLink® Afx Ø3.5 Locking Screw	18mm
P73 ST120	CoLink® Afx Ø3.5 Locking Screw	20mm
P73 ST122	CoLink® Afx Ø3.5 Locking Screw	22mm
P73 ST124	CoLink® Afx Ø3.5 Locking Screw	24mm
P73 ST126	CoLink® Afx Ø3.5 Locking Screw	26mm
P73 ST128	CoLink® Afx Ø3.5 Locking Screw	28mm
P73 ST130	CoLink® Afx Ø3.5 Locking Screw	30mm
P73 ST132	CoLink® Afx Ø3.5 Locking Screw	32mm
P73 ST134	CoLink® Afx Ø3.5 Locking Screw	34mm
P73 ST136	CoLink® Afx Ø3.5 Locking Screw	36mm
P73 ST138	CoLink® Afx Ø3.5 Locking Screw	38mm
P73 ST140	CoLink® Afx Ø3.5 Locking Screw	40mm
P73 ST142	CoLink® Afx Ø3.5 Locking Screw	42.5mm
P73 ST145	CoLink® Afx Ø3.5 Locking Screw	45mm
P73 ST147	CoLink® Afx Ø3.5 Locking Screw	47.5mm
P73 ST150	CoLink® Afx Ø3.5 Locking Screw	50mm
P73 ST152	CoLink® Afx Ø3.5 Locking Screw	52.5mm
P73 ST155	CoLink® Afx Ø3.5 Locking Screw	55mm
P73 ST157	CoLink® Afx Ø3.5 Locking Screw	57.5mm
P73 ST160	CoLink® Afx Ø3.5 Locking Screw	60mm
P73 ST210	CoLink® Afx Ø3.5 VAL Screw	10mm
P73 ST212	CoLink® Afx Ø3.5 VAL Screw	12mm
P73 ST214	CoLink® Afx Ø3.5 VAL Screw	14mm
P73 ST216	CoLink® Afx Ø3.5 VAL Screw	16mm
P73 ST218	CoLink® Afx Ø3.5 VAL Screw	18mm
P73 ST220	CoLink® Afx Ø3.5 VAL Screw	20mm
P73 ST222	CoLink® Afx Ø3.5 VAL Screw	22mm
P73 ST224	CoLink® Afx Ø3.5 VAL Screw	24mm
P73 ST226	CoLink® Afx Ø3.5 VAL Screw	26mm
P73 ST228	CoLink® Afx Ø3.5 VAL Screw	28mm



CoLink® Afx 3.5mm Diameter Screws (Sold Separately)

CATALOG NO.	DESCRIPTION	LENGTH
P73 ST230	CoLink® Afx Ø3.5 VAL Screw	30mm
P73 ST232	CoLink® Afx Ø3.5 VAL Screw	32mm
P73 ST234	CoLink® Afx Ø3.5 VAL Screw	34mm
P73 ST236	CoLink® Afx Ø3.5 VAL Screw	36mm
P73 ST238	CoLink® Afx Ø3.5 VAL Screw	38mm
P73 ST240	CoLink® Afx Ø3.5 VAL Screw	40mm
P73 ST242	CoLink® Afx Ø3.5 VAL Screw	42.5mm
P73 ST245	CoLink® Afx Ø3.5 VAL Screw	45mm
P73 ST247	CoLink® Afx Ø3.5 VAL Screw	47.5mm
P73 ST250	CoLink® Afx Ø3.5 VAL Screw	50mm
P73 ST252	CoLink® Afx Ø3.5 VAL Screw	52.5mm
P73 ST255	CoLink® Afx Ø3.5 VAL Screw	55mm
P73 ST257	CoLink® Afx Ø3.5 VAL Screw	57.5mm
P73 ST260	CoLink® Afx Ø3.5 VAL Screw	60mm

CoLink® 4.5mm Diameter Screws (Sold Separately)

CATALOG NO.	DESCRIPTION	LENGTH
V45 ST616	CoLink® Ø4.5 Non-Locking Screw	16mm
V45 ST618	CoLink® Ø4.5 Non-Locking Screw	18mm
V45 ST620	CoLink® Ø4.5 Non-Locking Screw	20mm
V45 ST622	CoLink® Ø4.5 Non-Locking Screw	22mm
V45 ST624	CoLink® Ø4.5 Non-Locking Screw	24mm
V45 ST626	CoLink® Ø4.5 Non-Locking Screw	26mm
V45 ST628	CoLink® Ø4.5 Non-Locking Screw	28mm
V45 ST630	CoLink® Ø4.5 Non-Locking Screw	30mm
V45 ST632	CoLink® Ø4.5 Non-Locking Screw	32mm
V45 ST634	CoLink® Ø4.5 Non-Locking Screw	34mm
V45 ST636	CoLink® Ø4.5 Non-Locking Screw	36mm
V45 ST638	CoLink® Ø4.5 Non-Locking Screw	38mm
V45 ST640	CoLink® Ø4.5 Non-Locking Screw	40mm
V45 ST645	CoLink® Ø4.5 Non-Locking Screw	45mm
V45 ST650	CoLink® Ø4.5 Non-Locking Screw	50mm
V45 ST655	CoLink® Ø4.5 Non-Locking Screw	55mm
V45 ST660	CoLink® Ø4.5 Non-Locking Screw	60mm
V45 ST665	CoLink® Ø4.5 Non-Locking Screw	65mm
V45 ST670	CoLink® Ø4.5 Non-Locking Screw	70mm
V45 ST675	CoLink® Ø4.5 Non-Locking Screw	75mm
V45 ST680	CoLink® Ø4.5 Non-Locking Screw	80mm
V45 ST685	CoLink® Ø4.5 Non-Locking Screw	85mm
V45 ST690	CoLink® Ø4.5 Non-Locking Screw	90mm
V45 ST695	CoLink® Ø4.5 Non-Locking Screw	95mm
V45 ST600	CoLink® Ø4.5 Non-Locking Screw	100mm
V45 ST716	CoLink® Ø4.5 Locking Screw	16mm
V45 ST718	CoLink® Ø4.5 Locking Screw	18mm
V45 ST720	CoLink® Ø4.5 Locking Screw	20mm
V45 ST722	CoLink® Ø4.5 Locking Screw	22mm
V45 ST724	CoLink® Ø4.5 Locking Screw	24mm
V45 ST726	CoLink® Ø4.5 Locking Screw	26mm
V45 ST728	CoLink® Ø4.5 Locking Screw	28mm
V45 ST730	CoLink® Ø4.5 Locking Screw	30mm
V45 ST732	CoLink® Ø4.5 Locking Screw	32mm
V45 ST734	CoLink® Ø4.5 Locking Screw	34mm
V45 ST736	CoLink® Ø4.5 Locking Screw	36mm
V45 ST738	CoLink® Ø4.5 Locking Screw	38mm
V45 ST740	CoLink® Ø4.5 Locking Screw	40mm
V45 ST745	CoLink® Ø4.5 Locking Screw	45mm
V45 ST750	CoLink® Ø4.5 Locking Screw	50mm
V45 ST755	CoLink® Ø4.5 Locking Screw	55mm
V45 ST760	CoLink® Ø4.5 Locking Screw	60mm
V45 ST765	CoLink® Ø4.5 Locking Screw	65mm

CoLink® 4.5mm Diameter Screws (Sold Separately)



CATALOG NO.	DESCRIPTION	LENGTH
V45 ST816	CoLink® Ø4.5 VAL Screw	16mm
V45 ST818	CoLink® Ø4.5 VAL Screw	18mm
V45 ST820	CoLink® Ø4.5 VAL Screw	20mm
V45 ST822	CoLink® Ø4.5 VAL Screw	22mm
V45 ST824	CoLink® Ø4.5 VAL Screw	24mm
V45 ST826	CoLink® Ø4.5 VAL Screw	26mm
V45 ST828	CoLink® Ø4.5 VAL Screw	28mm
V45 ST830	CoLink® Ø4.5 VAL Screw	30mm
V45 ST832	CoLink® Ø4.5 VAL Screw	32mm
V45 ST834	CoLink® Ø4.5 VAL Screw	34mm
V45 ST836	CoLink® Ø4.5 VAL Screw	36mm
V45 ST838	CoLink® Ø4.5 VAL Screw	38mm
V45 ST840	CoLink® Ø4.5 VAL Screw	40mm
V45 ST845	CoLink® Ø4.5 VAL Screw	45mm
V45 ST850	CoLink® Ø4.5 VAL Screw	50mm
V45 ST855	CoLink® Ø4.5 VAL Screw	55mm
V45 ST860	CoLink® Ø4.5 VAL Screw	60mm
V45 ST865	CoLink® Ø4.5 VAL Screw	65mm

CoLink® 5.0mm Diameter Cancellous Screws (Sold Separately)



CATALOG NO.	DESCRIPTION	LENGTH
V50 ST016	CoLink® Ø5.0 Cancellous Screw	16mm
V50 ST018	CoLink® Ø5.0 Cancellous Screw	18mm
V50 ST020	CoLink® Ø5.0 Cancellous Screw	20mm
V50 ST022	CoLink® Ø5.0 Cancellous Screw	22mm
V50 ST024	CoLink® Ø5.0 Cancellous Screw	24mm
V50 ST026	CoLink® Ø5.0 Cancellous Screw	26mm
V50 ST028	CoLink® Ø5.0 Cancellous Screw	28mm
V50 ST030	CoLink® Ø5.0 Cancellous Screw	30mm
V50 ST032	CoLink® Ø5.0 Cancellous Screw	32mm
V50 ST034	CoLink® Ø5.0 Cancellous Screw	34mm
V50 ST036	CoLink® Ø5.0 Cancellous Screw	36mm
V50 ST038	CoLink® Ø5.0 Cancellous Screw	38mm
V50 ST040	CoLink® Ø5.0 Cancellous Screw	40mm
V50 ST045	CoLink® Ø5.0 Cancellous Screw	45mm
V50 ST050	CoLink® Ø5.0 Cancellous Screw	50mm
V50 ST055	CoLink® Ø5.0 Cancellous Screw	55mm
V50 ST060	CoLink® Ø5.0 Cancellous Screw	60mm
V50 ST065	CoLink® Ø5.0 Cancellous Screw	65mm

CoLag® 6.7mm Diameter Compression Screws (Sold Separately)



CATALOG NO.	DESCRIPTION	LENGTH
P65 ST630	CoLag® Ø6.7 Compression Screw	30mm
P65 ST632	CoLag® Ø6.7 Compression Screw	32mm
P65 ST634	CoLag® Ø6.7 Compression Screw	34mm
P65 ST636	CoLag® Ø6.7 Compression Screw	36mm
P65 ST638	CoLag® Ø6.7 Compression Screw	38mm
P65 ST640	CoLag® Ø6.7 Compression Screw	40mm
P65 ST642	CoLag® Ø6.7 Compression Screw	42.5mm
P65 ST645	CoLag® Ø6.7 Compression Screw	45mm
P65 ST647	CoLag® Ø6.7 Compression Screw	47.5mm
P65 ST650	CoLag® Ø6.7 Compression Screw	50mm
P65 ST652	CoLag® Ø6.7 Compression Screw	52.5mm
P65 ST655	CoLag® Ø6.7 Compression Screw	55mm
P65 ST657	CoLag® Ø6.7 Compression Screw	57.5mm
P65 ST660	CoLag® Ø6.7 Compression Screw	60mm
P65 ST662	CoLag® Ø6.7 Compression Screw	62.5mm
P65 ST665	CoLag® Ø6.7 Compression Screw	65mm
P65 ST667	CoLag® Ø6.7 Compression Screw	67.5mm
P65 ST670	CoLag® Ø6.7 Compression Screw	70mm
P65 ST672	CoLag® Ø6.7 Compression Screw	72.5mm
P65 ST675	CoLag® Ø6.7 Compression Screw	75mm
P65 ST677	CoLag® Ø6.7 Compression Screw	77.5mm
P65 ST680	CoLag® Ø6.7 Compression Screw	80mm
P65 ST682	CoLag® Ø6.7 Compression Screw	82.5mm
P65 ST685	CoLag® Ø6.7 Compression Screw	85mm
P65 ST687	CoLag® Ø6.7 Compression Screw	87.5mm
P65 ST690	CoLag® Ø6.7 Compression Screw	90mm
P65 ST695	CoLag® Ø6.7 Compression Screw	95mm
P65 ST700	CoLag® Ø6.7 Compression Screw	100mm
P65 ST705	CoLag® Ø6.7 Compression Screw	105mm
P65 ST710	CoLag® Ø6.7 Compression Screw	110mm
P65 ST715	CoLag® Ø6.7 Compression Screw	115mm
P65 ST830	CoLag® Ø6.7 Fully Threaded Screw	30mm
P65 ST832	CoLag® Ø6.7 Fully Threaded Screw	32mm
P65 ST834	CoLag® Ø6.7 Fully Threaded Screw	34mm
P65 ST836	CoLag® Ø6.7 Fully Threaded Screw	36mm
P65 ST838	CoLag® Ø6.7 Fully Threaded Screw	38mm
P65 ST840	CoLag® Ø6.7 Fully Threaded Screw	40mm
P65 ST842	CoLag® Ø6.7 Fully Threaded Screw	42.5mm
P65 ST845	CoLag® Ø6.7 Fully Threaded Screw	45mm
P65 ST847	CoLag® Ø6.7 Fully Threaded Screw	47.5mm
P65 ST850	CoLag® Ø6.7 Fully Threaded Screw	50mm
P65 ST852	CoLag® Ø6.7 Fully Threaded Screw	52.5mm
P65 ST855	CoLag® Ø6.7 Fully Threaded Screw	55mm
P65 ST857	CoLag® Ø6.7 Fully Threaded Screw	57.5mm
P65 ST860	CoLag® Ø6.7 Fully Threaded Screw	60mm
P65 ST862	CoLag® Ø6.7 Fully Threaded Screw	62.5mm
P65 ST865	CoLag® Ø6.7 Fully Threaded Screw	65mm
P65 ST867	CoLag® Ø6.7 Fully Threaded Screw	67.5mm
P65 ST870	CoLag® Ø6.7 Fully Threaded Screw	70mm
P65 ST872	CoLag® Ø6.7 Fully Threaded Screw	72.5mm
P65 ST875	CoLag® Ø6.7 Fully Threaded Screw	75mm
P65 ST877	CoLag® Ø6.7 Fully Threaded Screw	77.5mm
P65 ST880	CoLag® Ø6.7 Fully Threaded Screw	80mm
P65 ST882	CoLag® Ø6.7 Fully Threaded Screw	82.5mm
P65 ST885	CoLag® Ø6.7 Fully Threaded Screw	85mm
P65 ST887	CoLag® Ø6.7 Fully Threaded Screw	87.5mm
P65 ST890	CoLag® Ø6.7 Fully Threaded Screw	90mm
P65 ST895	CoLag® Ø6.7 Fully Threaded Screw	95mm
P65 ST900	CoLag® Ø6.7 Fully Threaded Screw	100mm
P65 ST905	CoLag® Ø6.7 Fully Threaded Screw	105mm
P65 ST910	CoLag® Ø6.7 Fully Threaded Screw	110mm
P65 ST915	CoLag® Ø6.7 Fully Threaded Screw	115mm

CoLink® NeoFuse

MIS Plating System

CoLink® NeoFuse MIS Plates (Sold Separately)

CATALOG NO.	DESCRIPTION
P20 ST101	CoLink® NeoFuse MIS Plate, Standard
P20 ST201	CoLink® NeoFuse MIS Plate, 3.5mm Talar Holes



(Standard) (3.5mm Talar Holes)

Sterile-Packaged, Single-Use Instruments (Sold Separately)

CATALOG NO.	DESCRIPTION
P02 S0121	K-wire, Single Trocar 0.079 X 9"
P02 S0131	Olive Wire, 0.062x2.4"
P02 S0161	4.5x120mm Drill
P02 S0141	3.2x130mm Drill
P07 S0031	2.5x60mm Drill
P02 S0151	T20 Driver, AO
P07 S0041	T15 Driver, AO



In2Bones USA
6000 Poplar Ave., Suite 115
Memphis, TN 38119
844 602 6637
www.conmed.com/in2bones

In2Bones SAS
28, chemin du Petit Bois
69130 Ecully
France
+33 (0)4 72 29 26 26

CONMED Corporation
11311 Concept Blvd
Largo, FL 33773
USA

™ and © denote Trademarks and Registered Trademarks of CONMED or its affiliates. Patent pending.
©2025 CONMED Corporation. All Rights Reserved.

All content contained herein is furnished for informational purposes only. CONMED does not recommend a particular surgical product or procedure suitable for all patients. Each surgeon must evaluate the appropriateness of a device and corresponding techniques based on medical training, clinical judgment and surgical experience. The proper surgical technique and/or procedure are the responsibility of the medical professional. Indications, contraindications, warnings, and precautions are listed in the implant package insert and should be reviewed carefully by the physician and operating room personnel prior to any proposed procedure. Availability of these products might vary from a given country or region to another as a result of specific local regulatory approval or clearance requirements for sale in such country or region.

CAUTION: Federal law (USA) restricts this device to sale and use by, or on the order of a physician.

SP-22006-01 Rev. A 01/25